

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

APR 20 2010

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130133 ✓
A	Name	BRYAN BARLOW	ID# 4548 Date 4/16/10 ✓
	Agency	Alaska State Troopers	Phone # 907-783-0972
	Instrument Location	Girdwood ✓	
B	Alco S/N	X172966 ✓	Target Value .084 ✓ High Pressure 975
	Alco Test Value Average	.082 ✓	.085 ✓
		1 st Alco	2 nd Alco
Signature		Bryan Barlow ✓	
		(OVER)	


CAB
4/15/10
4/20/10


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (Do Not write in the area below)
- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
 - (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
 - (3) I am the Scientific Director of the State Breath Alcohol Program.
 - (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
 - (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
 - (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 26th day of April, 2010.

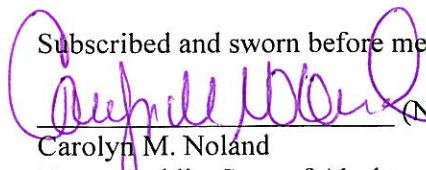
(Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130133

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130133

APRIL 16, 2010

OPERATOR'S NAME:

BARLOW BRYAN W

OPERATOR'S NUMBER: 4548

SUBJECT'S LAST NAME:

CALIBRATION

SUBJECT'S FIRST NAME/MI :

VERIFICATION OF

O.L. #: 1234567

DEPT/AGENCY: GOWO

CASE/REPORT: 10-00000

TEST TYPE: V

ALCO TARGET VALUE: .004

ALCO S/N: X172966

--- BREATH ANALYSIS ---

.004 ADJUSTED FOR 30.12 in		
ALCO TARGET	.004	19:34
BLANK TEST	.000	19:35
INTERNAL STANDARD	VERIFIED	19:35
ALCO TV 30.12 in	.002	19:35
BLANK TEST	.000	19:36
SUBJECT SAMPLE	.000	19:37
BLANK TEST	.000	19:37
ALCO TV 30.11 in	.005	19:38
BLANK TEST	.000	19:39

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130133

APRIL 16, 2010

TIME 19:31

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	41c
BAROMETER:	30.12 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

! " # \$ % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~ ¡ ¢